

FIG 1  
PRIOR ART

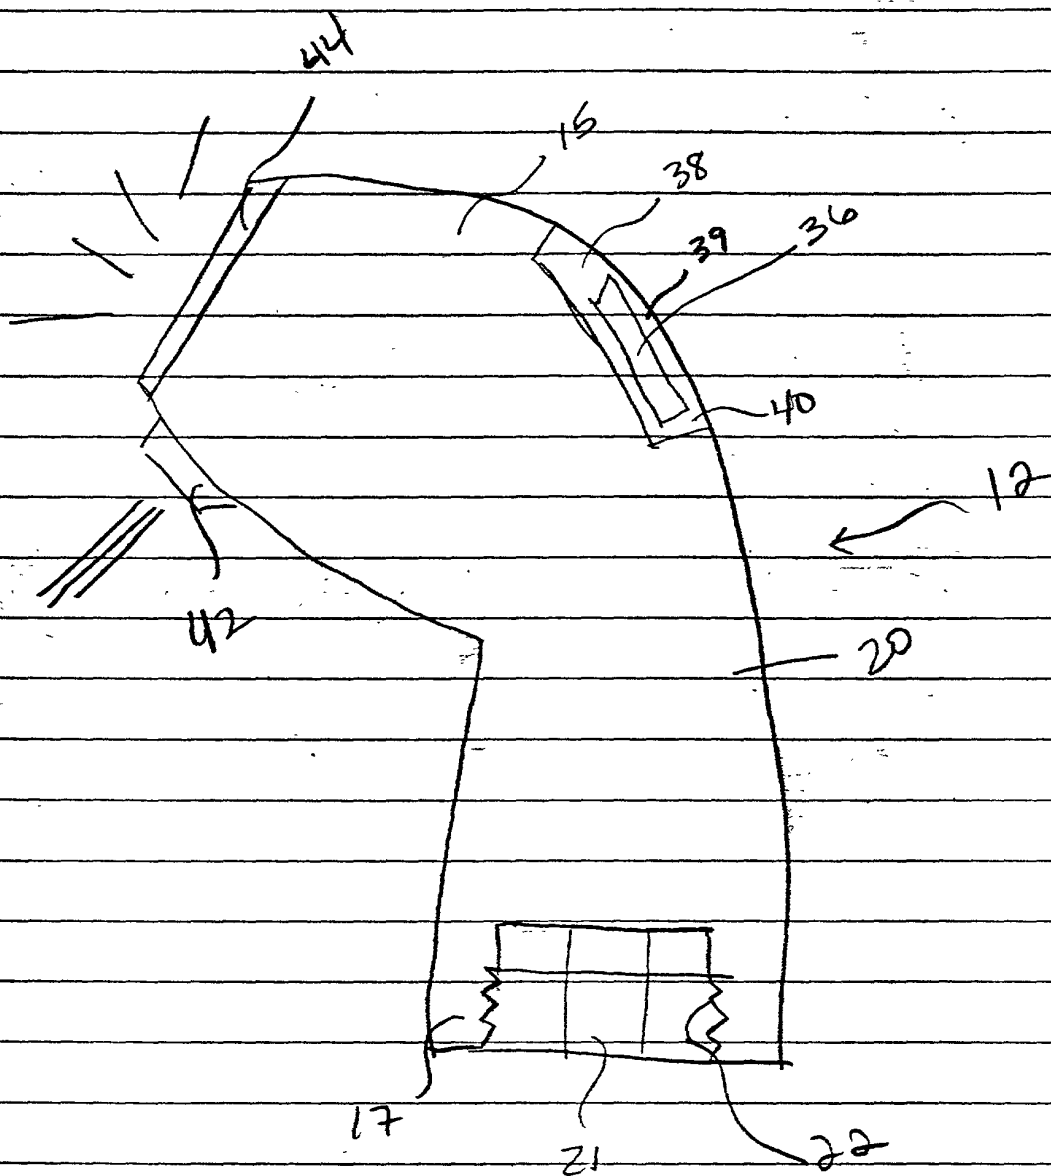


FIG. 2

PRIOR ART

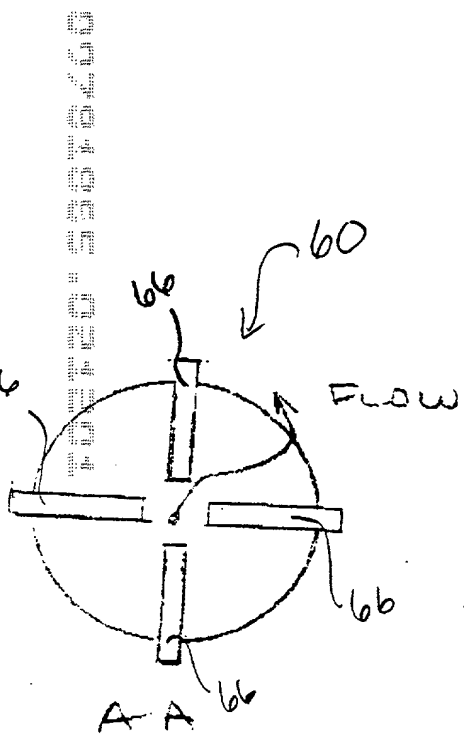


FIG 3.B

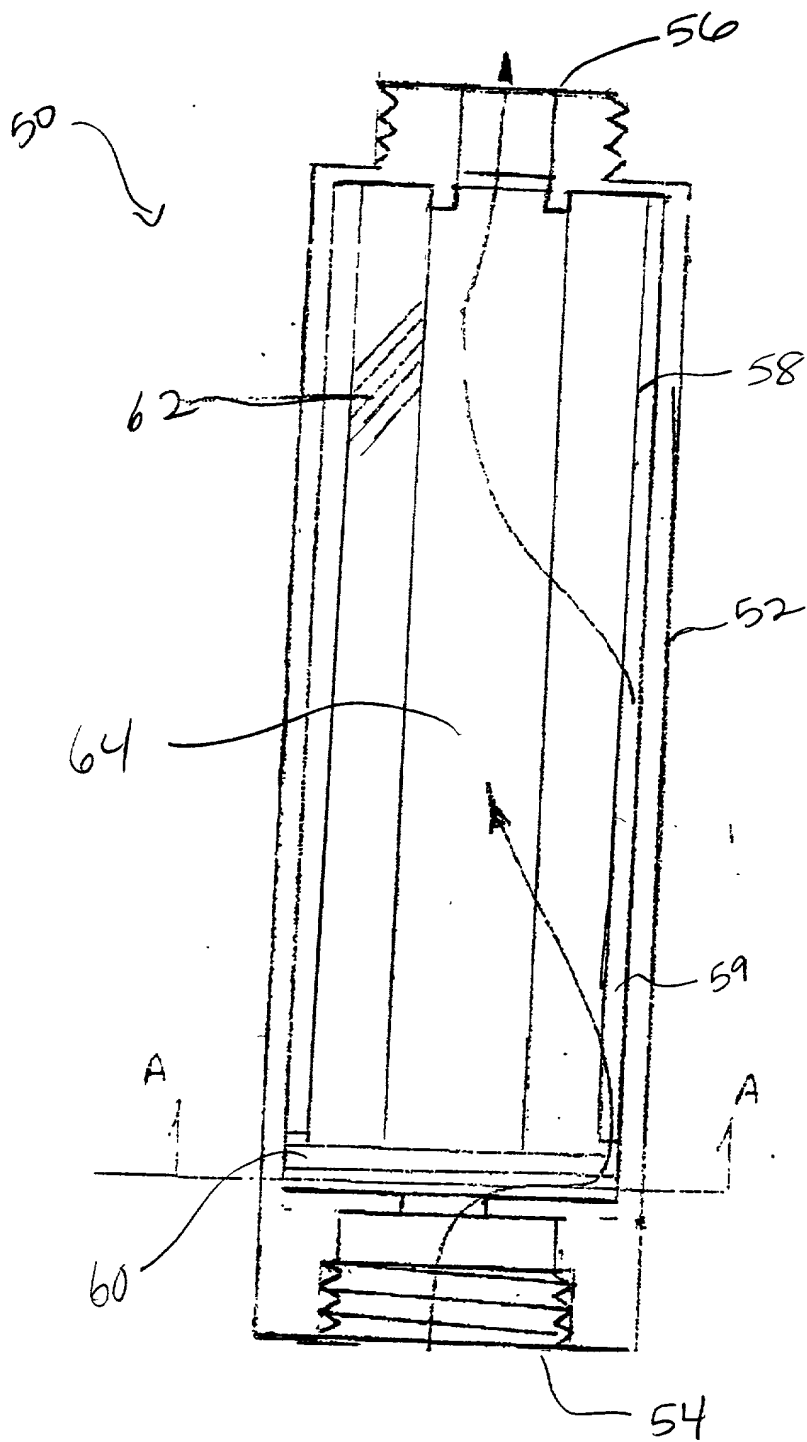


FIG 3A

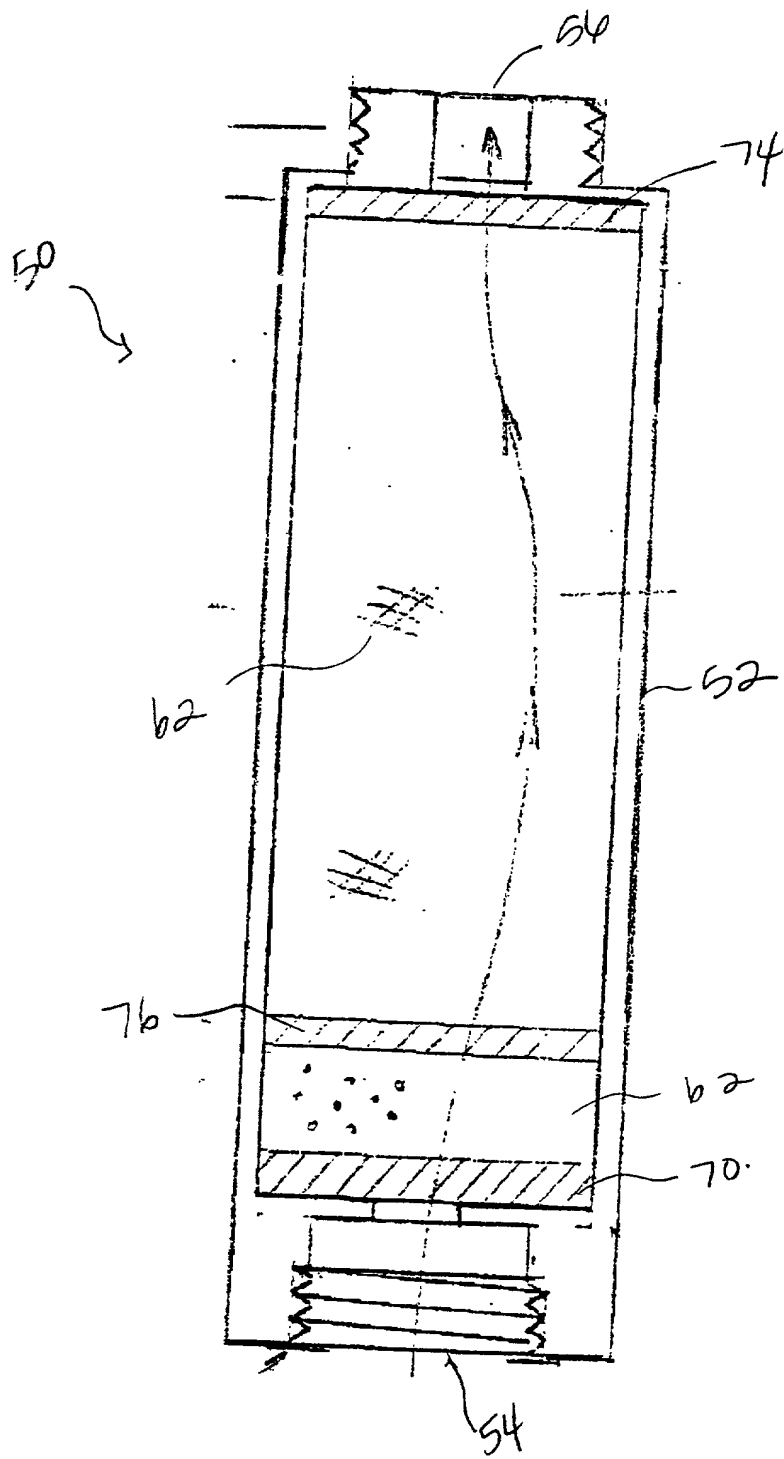


FIG 4

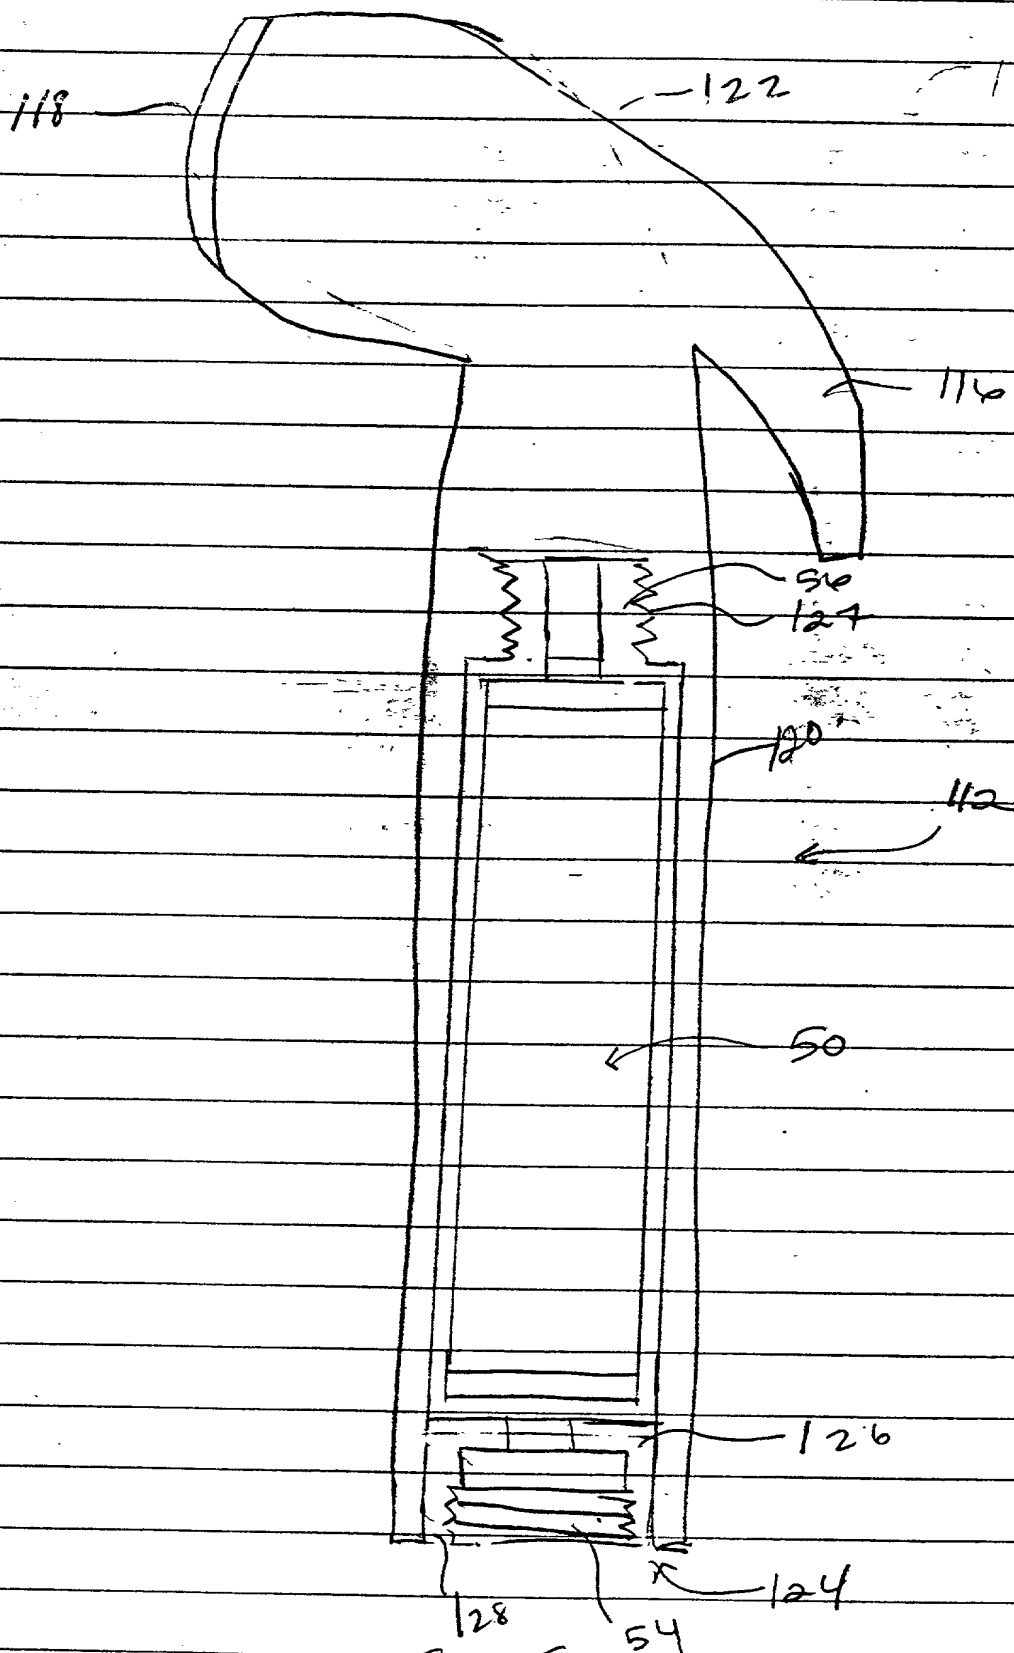


FIG 5

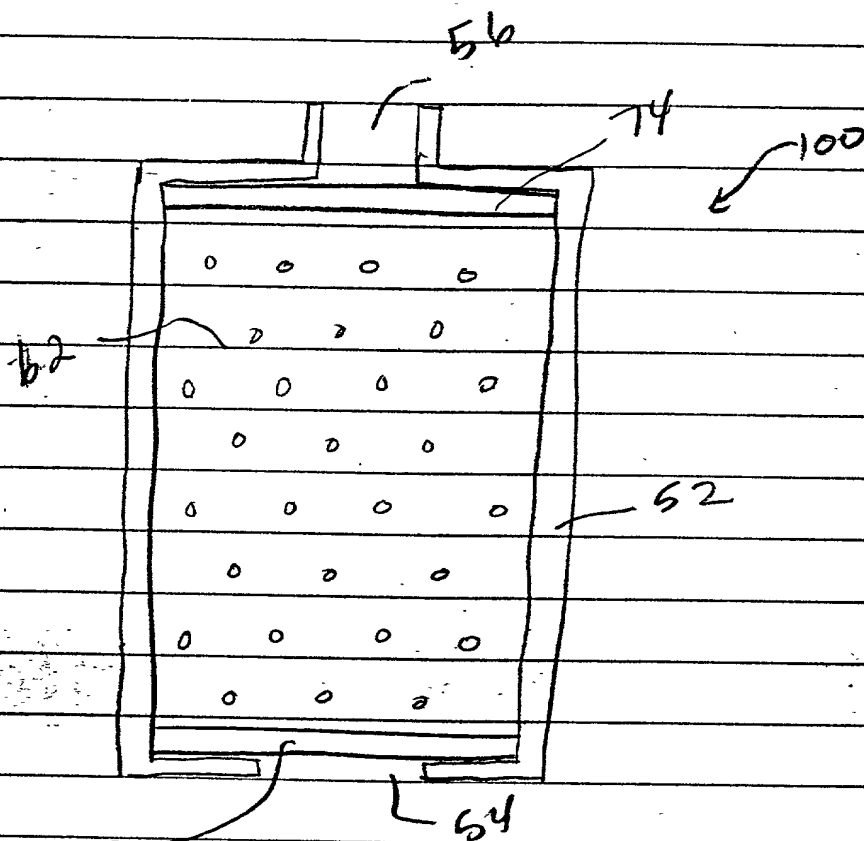


FIG. 6

40 ~>

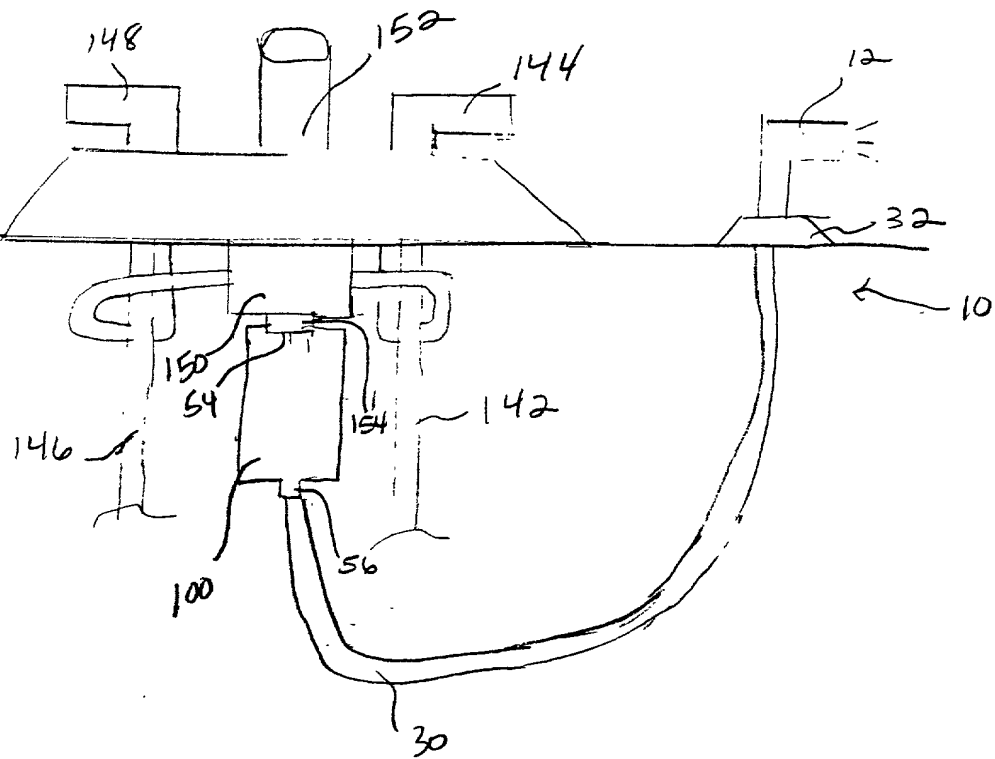


FIG. 7

FIG. 8A

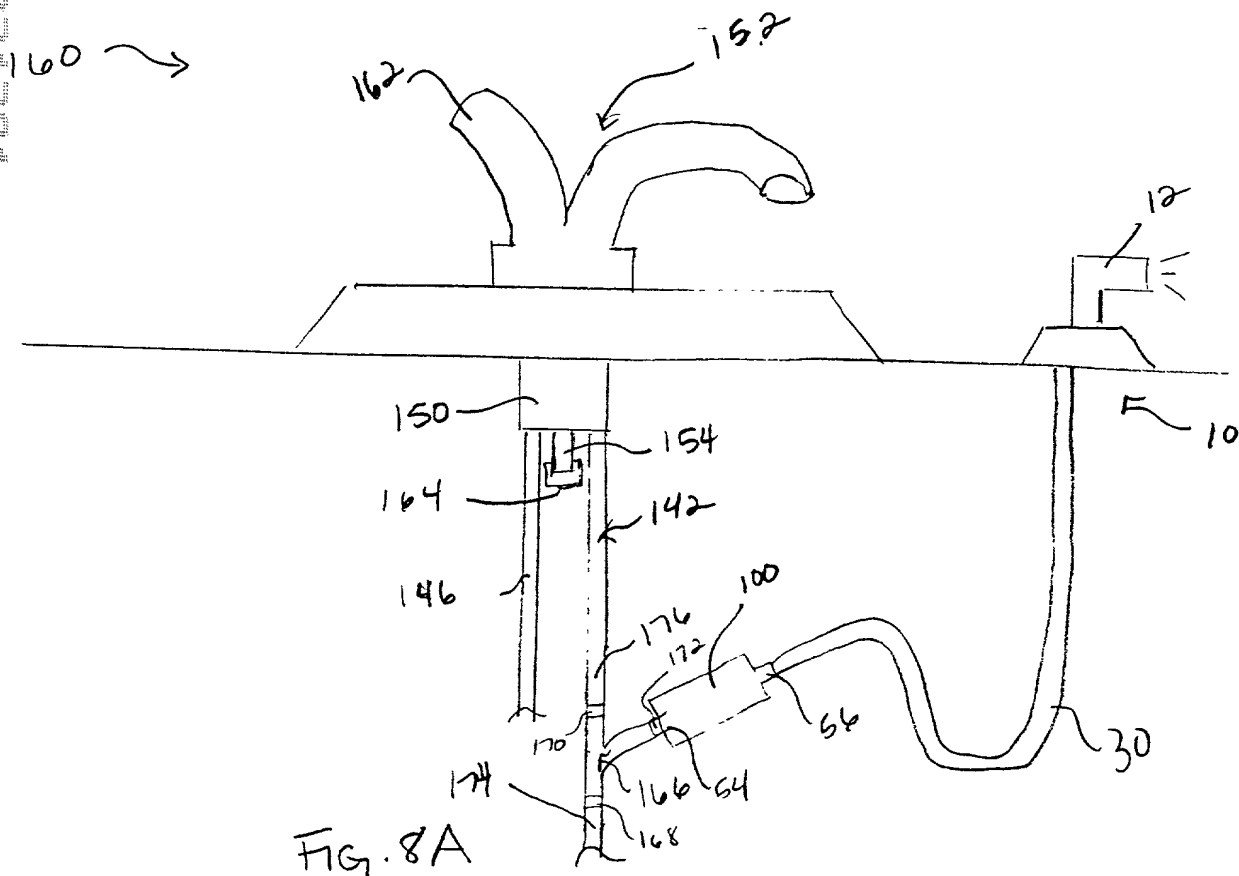


FIG. 8A

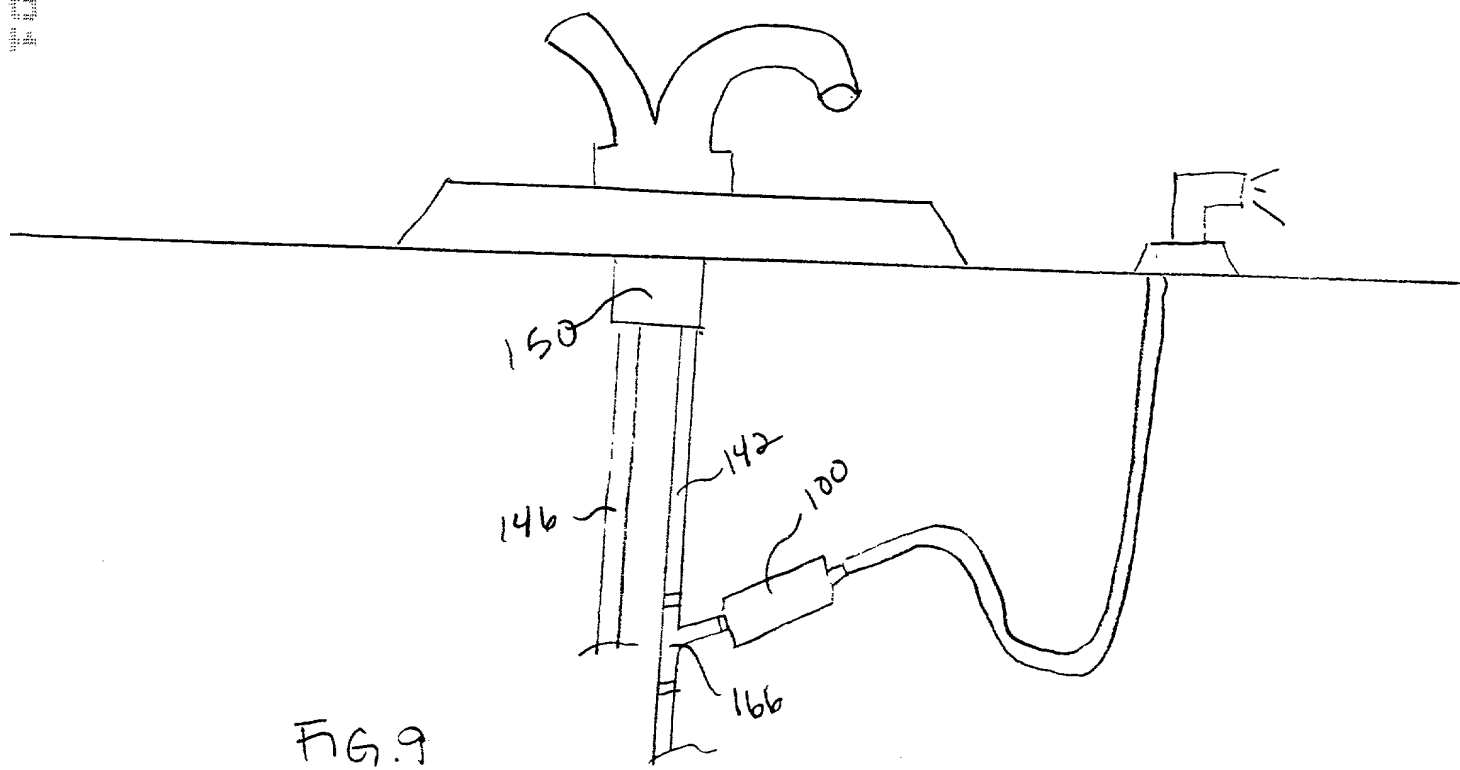
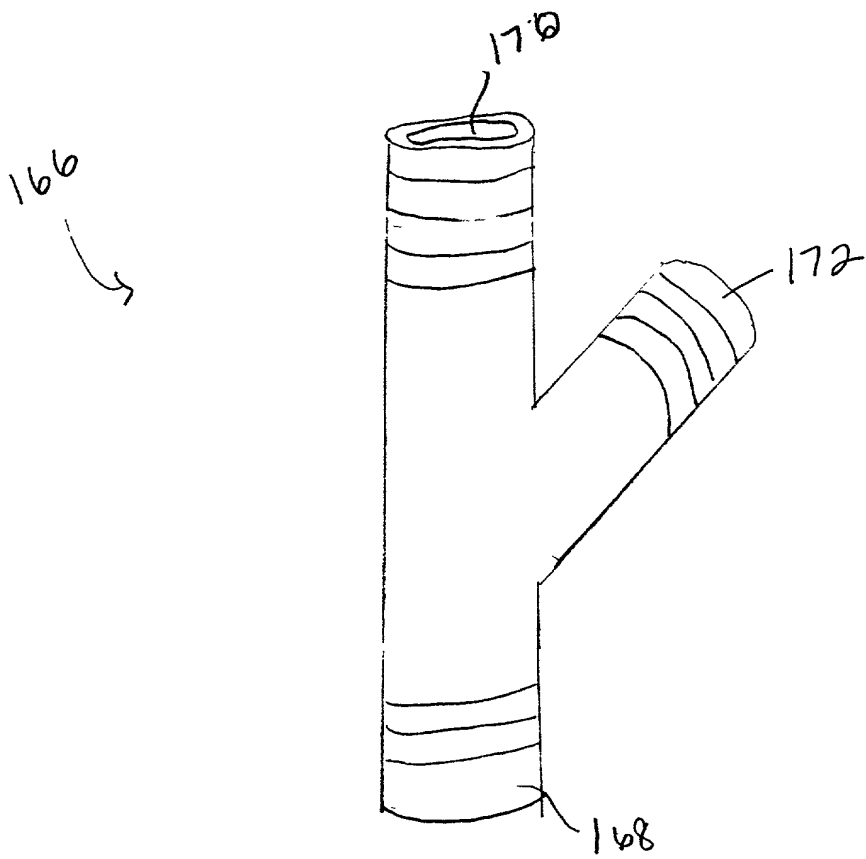




FIG. 10 is a cross-sectional view of the device 10 in a closed position.

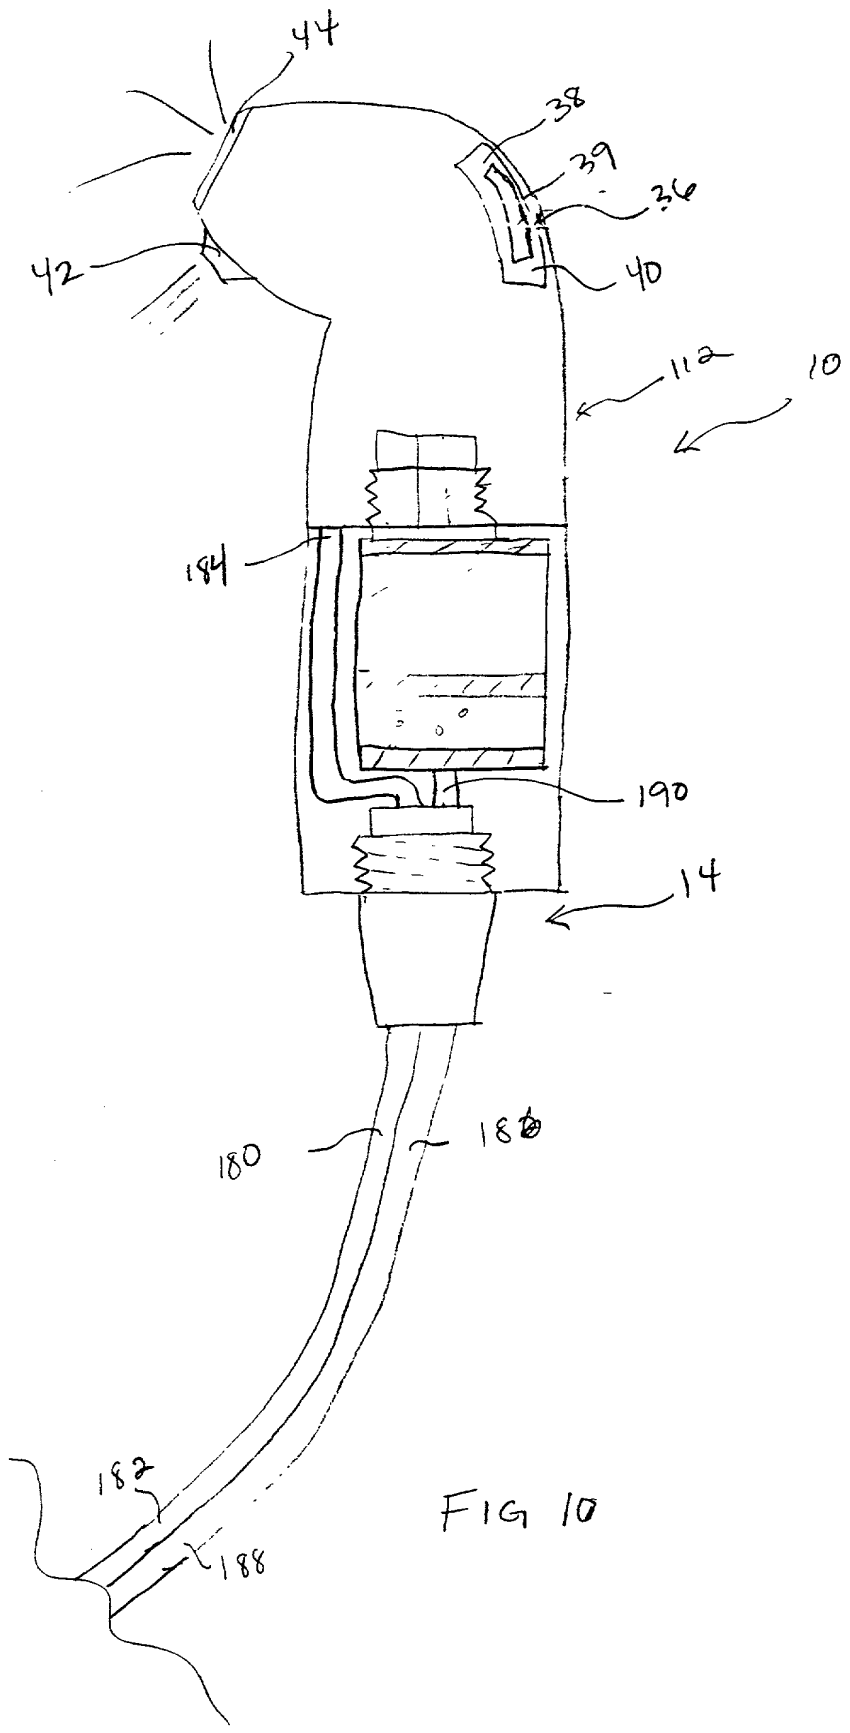


FIG 10

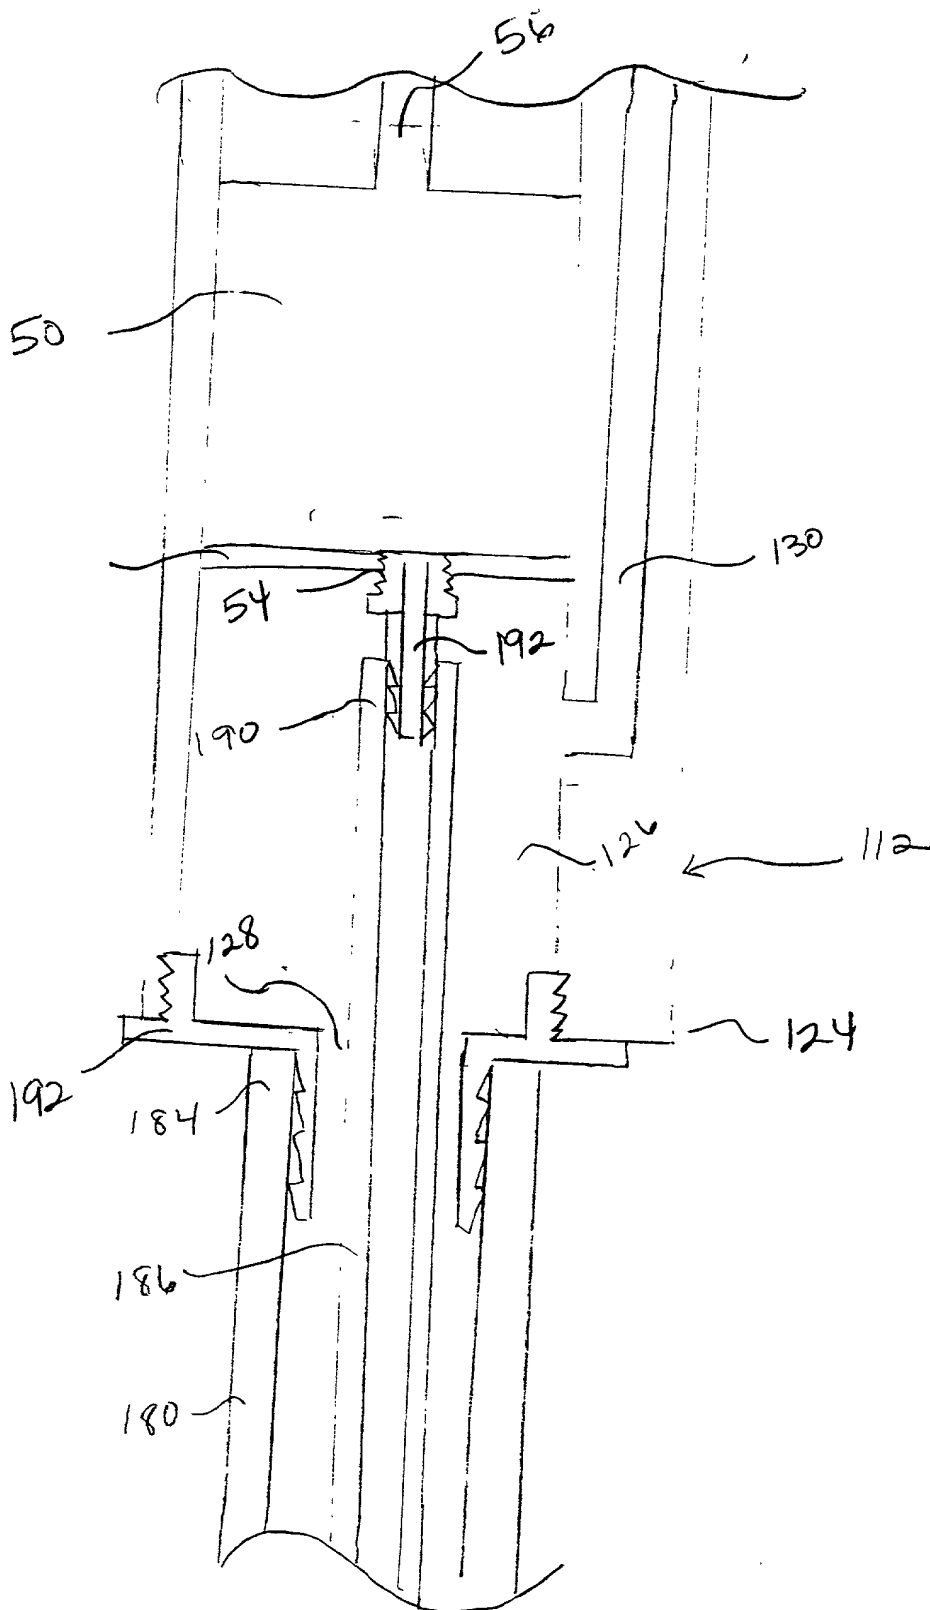


FIG. 11A

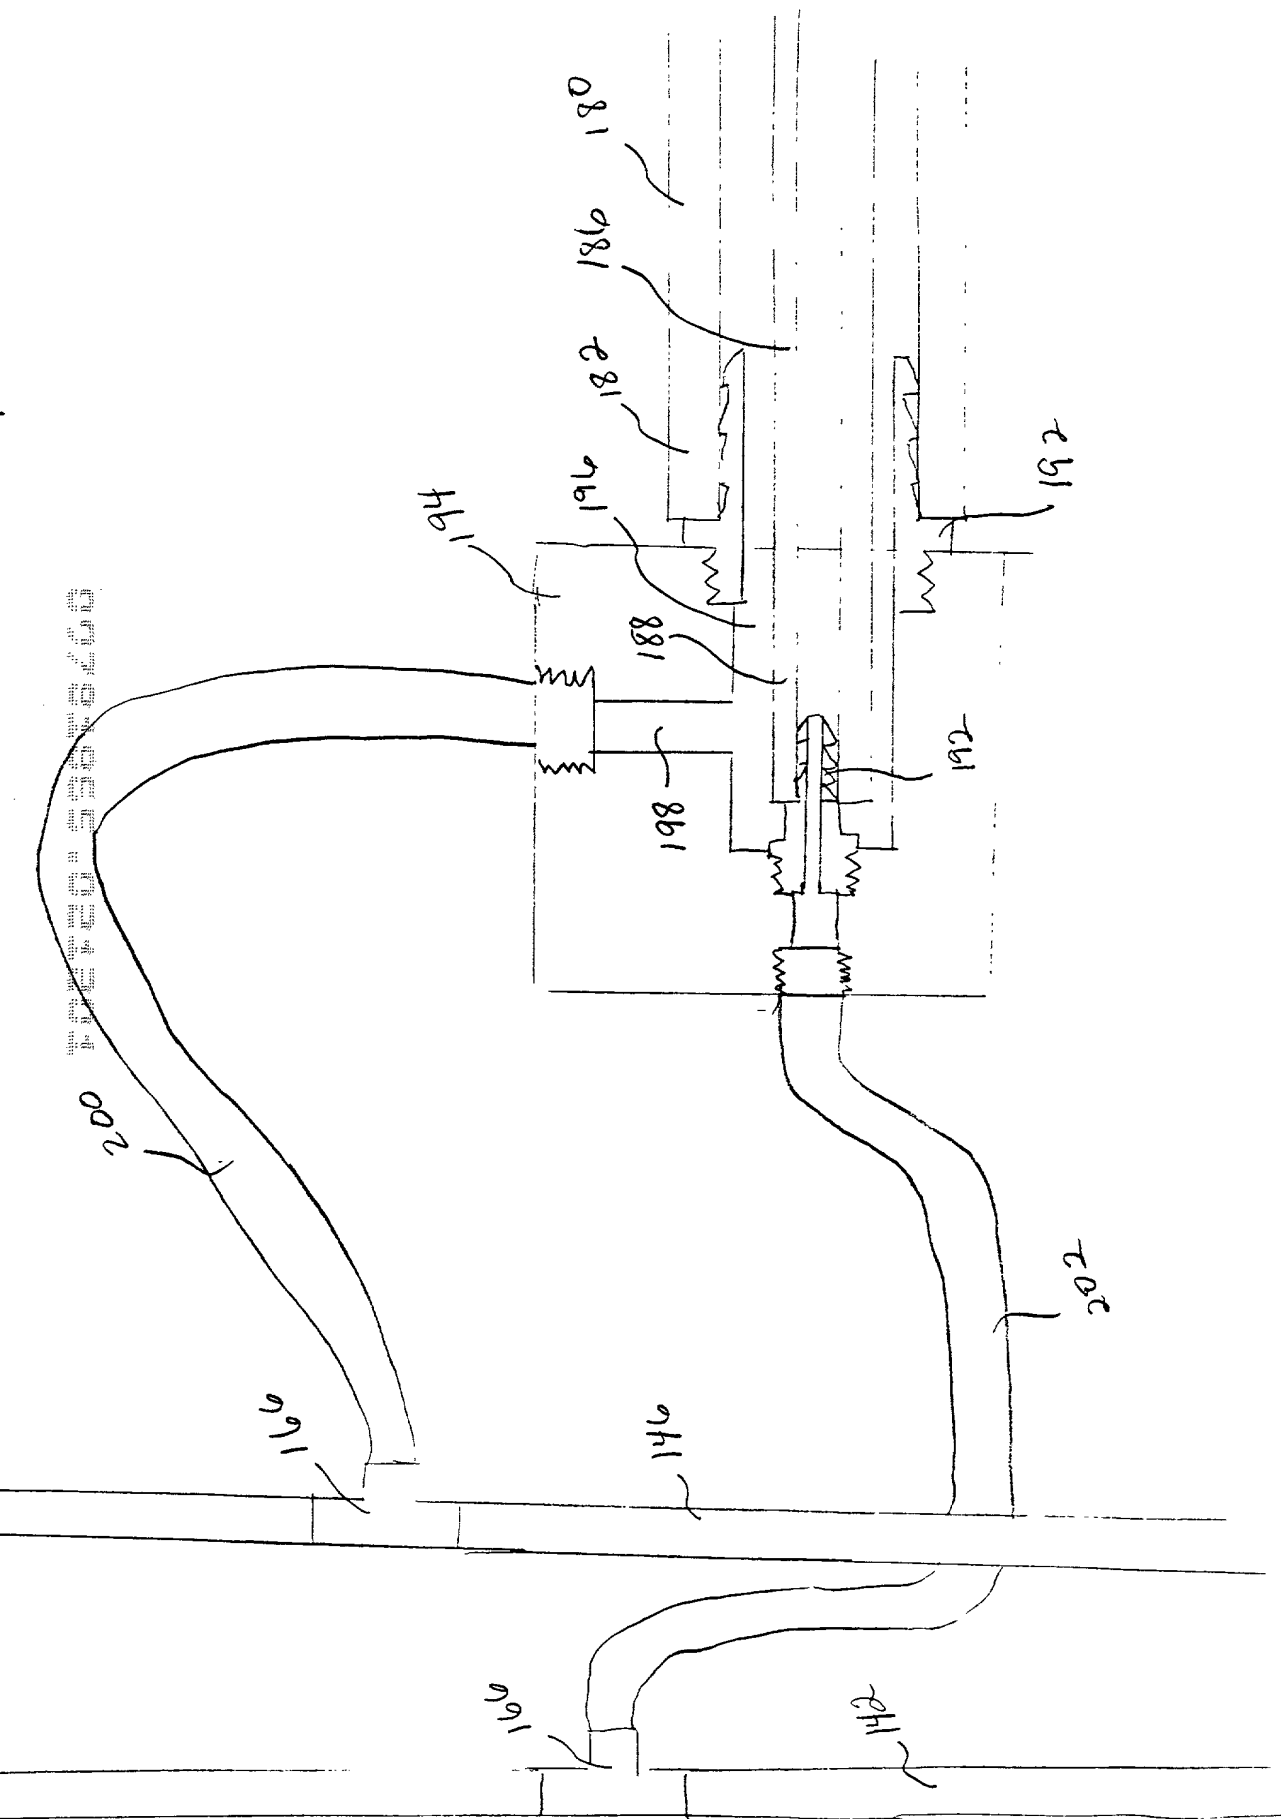


FIG. 11B

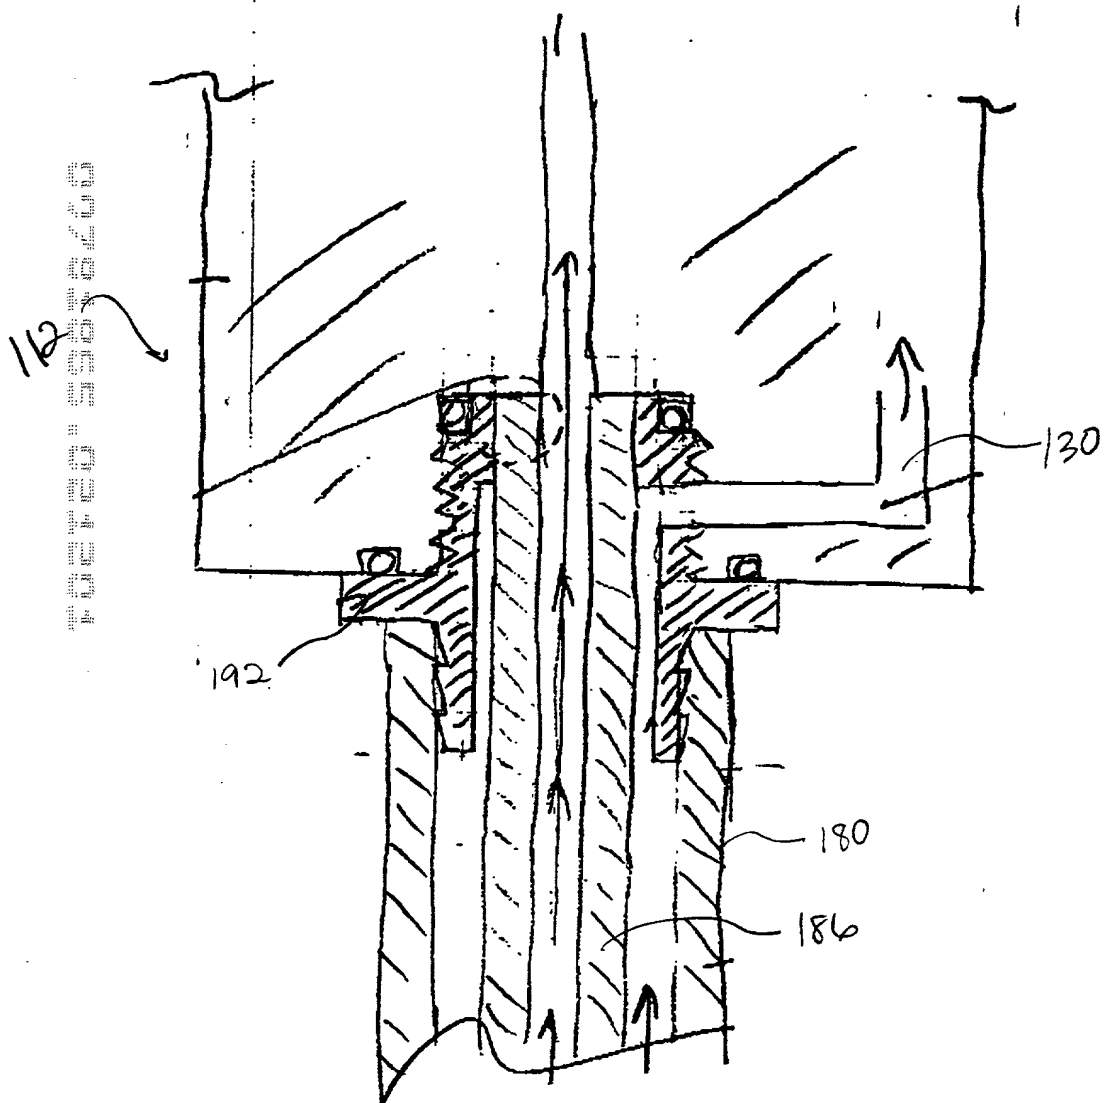


Fig. 11C